

Air velocity & IAQ measuring instruments

- testo 440 air velocity & IAQ measuring instrument
- testo 440 dP air velocity & IAQ measuring instrument incl. differential pressure

Intuitive: clearly structured measurement menus for the most important applications stored on the instrument


Wireless: Bluetooth probes for greater measuring convenience and a reduced tangle of cables in the case

Space-saving: a universal handle for all probes

Clear overview: parallel display of 3 measuring values; configuration and results at a glance

Reliable: internal memory for up to 7500 measurement protocols, USB interface for data export and optional printout of measuring values







The testo 440 combines the benefits of a compact handheld device with intuitive measurement menus and a comprehensive selection of air velocity & IAQ probes. This means you have all measuring tasks on air conditioning and ventilation systems reliably under control.

You can connect the testo 440 air velocity & IAQ measuring instrument either to a large selection of digital probes, the Testo Smart Probes or numerous Testo temperature probes. Clearly structured menus for measuring volume flow in ducts/at outlets, K-factor, degree of turbulence, cooling/heating load, mould indication and logging mode

are stored on the instrument. These menus enable you to accomplish the relevant measuring task more quickly, more efficiently and more reliably. Reports can be exported as Excel files via the USB interface or printed out on site.


The testo 440 air velocity & IAQ measuring instrument is available in two versions. The testo 440 dP model version also has an integrated differential pressure sensor. This makes measurements at filters as well as Pitot tube and K-factor measurements possible.



The testo 440 probe system

Completely versatile: a universal handle for all air velocity & IAQ probes. This saves space and reduces the weight, enabling you to perform accurate measurements in any application.


With the testo 440, you have all air conditioning and ventilation measurements systematically under control.

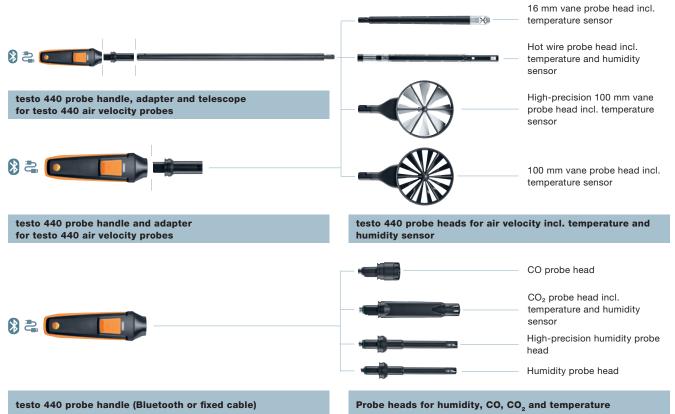

Advantages during measurement



All testo 440 air velocity probes for measurements in ducts have a scaled, extendible telescope (optionally extendible from 1 m to 2 m).



The 100 mm vane probe can be easily combined with the 90° angle and telescope, making measurements at ceiling outlets easier.




Do you need to carry out measurements in places where Bluetooth isn't possible? No problem: simply switch the probe head over from Bluetooth to the cable handle and you're ready.




With the testo 440 dP model, incl. differential pressure sensor, you can ensure that the filters in air conditioning systems are working properly and no contamination in the outdoor air gets into the indoor air.



Ordering data for testo 440

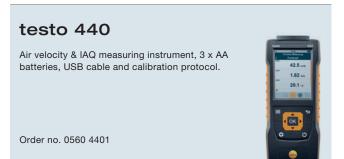

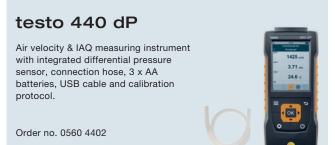

Technical data testo 440

	testo 440	testo 440 dP	
Temperature (NTC)			
Measuring range	-40 to -	+150 °C	
Accuracy (±1 digit)	±0.3 °C (-25 ±0.4 °C (+75	to -25.1 °C) to +74.9 °C) to +99.9 °C) aining meas. range)	
Resolution	0.1	°C	
Temperature (TC)			
Measuring range	-200 to -	⊦1370 °C	
Accuracy (±1 digit)	±(0.3 °C + 0	.3% of m.v.)	
Resolution	0.1	°C	
Differential pressure			
Measuring range		-150 to +150 hPa	
Accuracy (±1 digit)	-	±0.05 hPa (0 to +1.00 hPa) ±0.2 hPa + 1.5% of m.v. (+1.01 +150 hPa)	
Resolution		0.01 hPa	
Probe connections			
TC type K	1	х	
NTC TUC / digital probe with cable	1	х	
Bluetooth probe	•	etooth probe mart Probe	
Differential pressure	-	+	
Technical data			
Operating temperature	-20 to	+50 °C	
Storage temperature	-20 to +50 °C		
Battery type	3 x AA batteries		
Battery life	12 h (typically vane measurement)		
Weight	250 g		
Dimensions	154 x 65 x 32 mm		



The wired digital probes and the NTC probes of the testo 440 all have the practical TUC connection (**T**esto **U**niversal **C**onnector).



Ordering data for kits

Kits for measurement in ducts, at outlets and at filters

testo 440 delta P

Air Flow ComboKit 1 with BT

- testo 440 dP air velocity & IAQ measuring instrument incl. differential pressure with internal memory and data export function
- Universal probe handle with Bluetooth
- Hot wire probe head incl. temperature and humidity sensor
- 100 mm vane probe head incl. temperature sensor
- Telescope (1 m) and 90° angle to fit both probes
- Combi case for testo 440 dP and multiple probes



testo 440 delta P Air Flow ComboKit 2 with BT

- testo 440 dP air velocity & IAQ measuring instrument incl. differential pressure with internal memory and data export function
- Universal probe handle with Bluetooth
- 16 mm vane probe head incl. temperature sensor
- 100 mm vane probe head incl. temperature sensor
- Humidity probe head incl. temperature sensor
- Telescope (1 m) and 90° angle to fit both probes
- Combi case for testo 440 dP and multiple probes



Kits for measurements in ducts and at outlets

testo 440

Air Flow ComboKit 1 with BT

- testo 440 air velocity & IAQ measuring instrument with internal memory and data export function
- 100 mm vane probe with Bluetooth, incl. temperature sensor
- Hot wire probe with telescope (0.85 m) incl. temperature sensor, fixed cable (1.8 m) $\,$
- Measurement menu, e.g. for determining the volume flow
- Combi case for testo 440 and multiple probes



testo 440

Air Flow ComboKit 2 with BT

- testo 440 air velocity & IAQ measuring instrument with internal memory and data export function
- 100 mm vane probe with Bluetooth, incl. temperature sensor
- 16 mm vane probe with telescope (0.85 m), fixed cable (1.8 m)
- Measurement menu, e.g. for determining the volume flow
- Combi case for testo 440 and multiple probes





Ordering data for kits

Additional kits

testo 440 Hot Wire Kit - testo 440 air velocity & IAQ measuring instrument with internal memory and data export function - Hot wire probe incl. temperature sensor, fixed cable (1.8 m) with telescope (0.85 m) - Measurement menu, e.g. for determining the volume flow and timed and multi-point mean

testo 440

16 mm Vane Kit

- testo 440 air velocity & IAQ measuring instrument with internal memory and data export function
- Vane probe, fixed cable (1.8 m) with telescope (0.85 m)
- Measurement menu, e.g. for determining the volume flow and timed and multi-point mean calculation
- Basic case for testo 440 and 1 probe Order no. 0563 4401



testo 440

Order no. 0563 4400

calculation

100 mm Vane Kit with BT

- testo 440 air velocity & IAQ measuring instrument with internal memory and data export function
- 100 mm vane probe with Bluetooth, incl. temperature sensor
- Measurement menu, e.g. for determining the volume flow
- Basic case for testo 440 and 1 probe

- Basic case for testo 440 and 1 probe



Order no. 0563 4403

testo 440

Indoor Comfort ComboKit

with BT

- testo 440 air velocity & IAQ measuring instrument with internal memory and data export function
- Turbulence probe (400 mm)
- CO₂ probe with Bluetooth, incl. temperature and humidity sensor
- Combi case for testo 440 and multiple probes

Order no. 0563 4408



testo 440

CO₂ Kit with BT

- testo 440 air velocity & IAQ measuring instrument
- $\mathrm{CO_2}$ probe with Bluetooth, incl. temperature and humidity sensor
- Basic case for testo 440 and 1 probe



Order no. 0563 4405

testo 440

Humidity Kit with BT

- testo 440 air velocity & IAQ measuring instrument
- Humidity and temperature probe with Bluetooth
- Basic case for testo 440 and 1 probe



Order no. 0563 4404


testo 440

Lux Kit

- testo 440 air velocity & IAQ measuring instrument
- Lux probe
- Basic case for testo 440 and 1 probe



Order no. 0563 4402

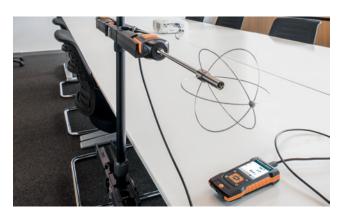



Digital air velocity probes

Probe type		Measuring range	Accuracy	Resolution	Order no.
Digital flow probes					
Hot wire probe with Bluetooth, incl. temperature and humidity sensor	570 to 1000 mm		±(0.03 m/s + 4% of m.v.) (0 to 20 m/s) ±(0.5 m/s + 5% of m.v.)		0635 1571
Hot wire probe, fixed cable, incl. temperature and humidity sensor	570 to 1000 mm 09 mm	0 to 50 m/s -20 to +70 °C 5 to +95% RH	(20.01 to 30 m/s) ±0.5 °C (0 to +70 °C) ±0.8 °C (-20 to 0 °C) ±3.0% RH (10 to 35% RH) ±2.0% RH (35 to 65% RH)	0.01 m/s 0.1 °C 0.1% RH	0635 1572
Hot wire probe head, incl. temperature and humidity sensor	230 mm		±3.0% RH (65 to 90% RH) ±5% RH (remaining meas. range)		0635 1570
Vane probe (Ø 16 mm) with Bluetooth, incl. temperature sensor	570 to 1000 mm				0635 9571
Vane probe (Ø 16 mm), fixed cable, incl. temperature sensor	570 to 1000 mm	0.6 to 50 m/s -10 to +70 °C	±(0.2 m/s + 1% of m.v.) (0.6 to 40 m/s) ±(0.2 m/s + 2% of m.v.) (40.1 to 50 m/s)	0.1 m/s 0.1 °C	0635 9572
Vane probe head (Ø 16 mm), incl. temperature sensor	230 mm — 210 mm — 210 mm		±1.8 °C		0635 9570
Hot wire probe, fixed cable, incl. temperature sensor	300 to 850 mm	0 to 30 m/s -20 to +70 °C	±(0.03 m/s + 4% of m.v.) (0 to 20 m/s) ±(0.5 m/s + 5% of m.v.) (20.01 to 30 m/s) ±0.5 °C	0.01 m/s 0.1 °C	0635 1032
Vane probe (Ø 16 mm) fixed cable	300 to 850 mm	0.6 to 50 m/s	±(0.2 m/s + 1% of m.v.) (0.6 to 40 m/s) ±(0.2 m/s + 2% of m.v.) (40.1 to 50 m/s)	0.1 m/s	0635 9532
Fume hood probe, fixed cable	150 mm — Ø 10 mm	0 to 5 m/s 0 to +50 °C	±(0.02 m/s + 5% of m.v.) (0 to 5 m/s) ±0.5 °C	0.01 m/s 0.1 °C	0635 1052
	large cross-section, we recommend a			'	
High-precision vane probe (Ø 100	extended to up to 2 m for all flow prob	es with an inte	erchangeable handle.		0635 9371
mm) with Bluetooth, including temperature sensor	9 100 mm				0000 007 1
High-precision vane probe (Ø 100 mm), fixed cable, incl. temperature sensor	Ø 100 mm	0.1 to 15 m/s -20 to +70 °C	±(0.1 m/s + 1.5% of m.v.) (0.1 to 15 m/s) ±0.5 °C	0.01 m/s 0.1 °C	0635 9372
High-precision vane probe head (Ø 100 mm), incl. temperature sensor	Ø 100 mm				0635 9370
Vane probe (Ø 100 mm) with Bluetooth, incl. temperature sensor	8 0 100 mm				0635 9431
Vane probe (Ø 100 mm) , fixed cable, incl. temperature sensor	Ø 100 mm	0.3 to 35 m/s -20 to +70 °C	°C (20.01 to 35 m/s)	0.01 m/s 0.1 °C	0635 9432
Vane probe head (Ø 100 mm), incl. temperature sensor	(§+≥1) 0 100 mm		±0.5 °C		0635 9430

¹⁾ For use with cable handle (order no. 0554 2222) or Bluetooth handle (order no. 0554 1111) in conjunction with adapter (order no. 0554 2160).

It can simply be fitted to the 100 mm vane probes.

For convenient ceiling measurements, the telescope with 90° angle (0550 0960) has been developed.



Other digital probes and probe accessories

Probe type		Measuring range	Accuracy	Resolution	Order no.
Digital humidity probes					
Humidity/temperature probe with Bluetooth	290 mm Ø 12 mm				0636 9731
Humidity/temperature probe, fixed cable	290 mm Ø 12 mm	0 to 100% RH -20 to +70 °C	±2% RH (5 to 90% RH) ±0.5 °C	0.1% RH 0.1 °C	0636 9732
Humidity/temperature probe head	8+2 140 mm				0636 9730
High-precision humidity/temperature probe with Bluetooth	290 mm Ø 12 mm		±(0.6% RH + 0.7% of m.v.)		0636 9771
High-precision humidity/temperature probe, fixed cable	290 mm Ø 12 mm	0 to 100% RH -20 to +70 °C	(0 to 90% RH) ±(1.0% RH + 0.7% of m.v.) (90 to 100% RH) ±0.3 °C (15 to 30 °C)	0.01% RH 0.1 °C	0636 9772
High-precision humidity/temperature probe head	3+ = 2) 140 mm Ø 12 mm		±0.5 °C (remaining meas. range)		0636 9770
Robust humidity/temperature probe for temperatures up to +180 °C, fixed cable	270 mm — Ø 12 mm	0 to 100% RH -20 to +180 °C	±3% RH (0 to 2% RH) ±2% RH (2.1 to 98% RH) ±3% RH (98.1 to 100% RH) ±0.5 °C (-20 to 0 °C) ±0.4 °C (0.1 to +50 °C) ±0.5 °C (+50.1 to +180 °C)	0.1% RH 0.1 °C	0636 9775
Digital comfort probes		,	1	'	,
Turbulence probe, fixed cable	190 mm	0 to +5 m/s 0 to +50 °C	±(0.03 m/s + 4% of m.v.) (0 to 5 m/s) ±0.5 °C	0.01 m/s 0.1 °C	0628 0152
Lux probe, fixed cable	110 mm 55 mm	0 to 100,000 lux	DIN EN 13032-1 Appendix B Class C according to DIN 5032-7	0.1 lux (< 10,000 lux) 1 lux (≥ 10,000 lux)	0635 0551
CO ₂ probe with Bluetooth, incl. temperature and humidity sensor	280 mm 30 mm		±(50 ppm + 3% of m.v.) (0 to 5000 ppm) ±(100 ppm + 5% of m.v.) (5001 to 10,000 ppm) ±3% RH (10 to 35% RH) ±2% RH (35 to 65% RH) ±3% RH (65 to 90% RH) ±5% RH (remaining meas. range) ±0.5 °C	1 ppm 0.1% RH 0.1 °C	0632 1551
CO ₂ probe, fixed cable, incl. temperature and humidity sensor	280 mm 30 mm	0 to 10,000 ppm CO ₂ 5 to +95% RH 0 to +50 °C			0632 1552
CO ₂ probe head, incl. temperature and humidity sensor	30 mm				0632 1550
CO probe with Bluetooth	30 mm				0632 1271
CO probe, fixed cable	200 mm 30 mm	0 to 500 ppm	±3 ppm (0 to 30 ppm) ±10% of m.v. (30.1 to 500 ppm)	0.1 ppm	0632 1272
CO probe head	30 mm 30 mm				0632 1270
Probe handle and adapter					
Cable handle for connecting testo 440 probe heads					0554 2222
Bluetooth handle for connecting testo 440 probe heads	8				0554 1111
Handle adapter for connecting testo 440 flow probes		─			0554 2160

²⁾ For use with cable handle (order no. 0554 2222) or Bluetooth handle (order no. 0554 1111).



Testo Smart Probes

Testo Smart Probes		Measuring range	Accuracy ±1 digit	Res- olution	Order no.
Temperature		'			
testo 115i Clamp thermometer with smartphone operation, for measurements on pipelines with diameters of 6 to maximum 35 mm, incl. batteries and calibration protocol	8	-40 to +150 °C	±1.3 °C (-20 to +85 °C)	0.1 °C	0560 1115
testo 905i Thermometer with smartphone operation, including batteries and calibration protocol	*	-50 to +150 °C	±1 °C	0.1 °C	0560 1905
testo 805i Infrared thermometer with smartphone operation, including batteries and calibration protocol		-30 to +250 °C	±1.5 °C or ±1.5% of m.v. (0 to +250 °C) ±2.0 °C (-20 to -0.1 °C) ±2.5 °C (-30 to -20.1 °C)	0.1 °C	0560 1805
Humidity					
testo 605i Thermohygrometer with smartphone operation, including batteries and calibration protocol	8	0 to 100% RH -20 to +60 °C	±(1.8% RH + 3% of m.v.) at +25 °C (5 to 80% RH) ±0.8 °C (-20 to 0 °C) ±0.5 °C (0 to +60 °C)	0.1% RH 0.1 °C	0560 1605
Flow					
testo 405i Thermal anemometer with smartphone operation, telescopic tube extendible to up to 400 mm, incl. batteries and calibration protocol	*	0 to 30 m/s -20 to +60 °C	±(0.1 m/s + 5% of m.v.) (0 to 2 m/s) ±(0.3 m/s + 5% of m.v.) (2 to 15 m/s) ±0.5 °C	0.01 m/s 0.1 °C	0560 1405
testo 410i Vane anemometer with smartphone operation, including batteries and calibration protocol	*	0.4 to 30 m/s -20 to +60 °C	±(0.2 m/s + 2% of m.v.) (0.4 to 20 m/s) ±0.5 °C	0.1 m/s 0.1 °C	0560 1410
Pressure					
testo 510i Differential pressure measuring instrument with smartphone operation, including hose set (Ø 4 mm and 5 mm) with adapter, batteries and calibration protocol	3	-150 to 150 hPa	±0.05 hPa (0 to 1 hPa) ±(0.2 hPa + 1.5% of m.v.) (1 to 150 hPa)	0.01 hPa	0560 1510
testo 549i High-pressure measuring instrument with smartphone operation, including batteries and calibration protocol	8	-1 to 60 bar	0.5% of final value	0.01 bar	0560 1549



Analogue temperature probes

Probe type	Dimensions Probe shaft/probe shaft	tip	Measuring range	Accuracy	t ₉₉	Order no.
Watertight immersion/penetration	115 mm	50 mm	-50 to +150 °C	±0.5% of m.v.	10 s	0615 1212
probe NTC, fixed cable 1.2 m	Ø 5 mm	Ø 4 mm		(+100 to +150 °C) ±0.2 °C (-25 to +74.9 °C) ±0.4 °C (remaining meas. range)		
Robust air probe, NTC, fixed cable 1.2 m	115 mm	50 mm	-50 to +125 °C	±0.2 °C (-25 to +80 °C) ±0.4 °C (remaining meas. range)	60 s	0615 1712
Clamp probe for magaziramenta en	Ø 5 mm	Ø 4 mm	-40 to +125 °C	±1 °C (-20 to +85 °C)	60 s	0615 5505
Clamp probe for measurements on pipes from 6 to 35 mm diameter, NTC, fixed cable 1.5 m	x 0		-40 10 +125 0	±1 0 (-20 to +03 0)	003	0013 3303
Robust air probe, TC type K, fixed cable	115 mm		-60 to +400 °C	Class 2 1)	200 s	0602 1793
	Ø 4 mm					
Fast-reaction surface probe with sprung thermocouple strip, also	115 mm		-60 to +300 °C	Class 2 1)	3 s	0602 0393
suitable for non-plane surfaces,	0					
measuring range briefly up to +500 °C, TC type K, fixed cable	Ø 5 mm	Ø 12 mm				
Fast-reaction paddle surface probe,	145 mm	_ 40 mm	0 to +300 °C	Class 2 1)	5 s	0602 0193
for measurements in places that are difficult to access, e.g. narrow	143 11111					
openings and cracks, TC type K, fixed cable	Ø 8 mm	Ø 7 mm				
Precise, watertight surface probe	150 mm		-60 to +1000 °C	Class 1 1)	20 s	0602 0693
with small measuring head for plane surfaces, TC type K, fixed cable	Ø 2.5 mm	Ø 4 mm				
	Ø 2.5 mm	Ø 4 mm				
Fast-reaction surface probe with sprung thermocouple strip, angled for non-plane surfaces as well, measuring range briefly up to	80 mm Ø 5 mm	Ø 12 mm	-60 to +300 °C	Class 2 1)	3 s	0602 0993
+500 °C, TC type K, fixed cable	ν					
Surface temperature probe TC type	985 ±5 mm	12 mm	-50 to +250 °C	Class 2 1)	3 s	0602 2394
K, with telescope max. 985 mm, for measurements in places that are						
difficult to access, fixed cable 1.6 m (correspondingly shorter when telescope is extended)		Ø 25 mm				
Magnetic probe, adhesive power	35 mm		-50 to +170 °C	Class 2 1)	150 s	0602 4792
approx. 20 N, with magnets, for measurements on metal surfaces, TC type K, fixed cable	Ø 20 mm					
Magnetic probe, adhesive power	75 mm		-50 to +400 °C	Class 2 1)		0602 4892
approx. 10 N, with magnets, for higher temperatures, for measurements on metal surfaces, TC type K, fixed cable	Ø 21 mm					

¹⁾ According to standard EN 60584-2, the accuracy of Class 1 refers to -40 to +1000 °C (type K), Class 2 to -40 to +1200 °C (type K), Class 3 to -200 to +40 °C (type K). A probe only ever complies with one accuracy class.

Information about surface measurement:

- The specified response times t_{99} are measured on polished steel or aluminium plates at +60 °C. The specified accuracies are sensor accuracies.
- Accuracy in your application depends on the surface properties (roughness), the material of the measurement object (thermal capacity and heat transfer) and the sensor accuracy. Testo will produce a corresponding calibration certificate for the deviations of your measurement system in your application. For this, Testo uses a surface test bed developed in cooperation with the PTB (Physikalisch Technische Bundesanstalt National Metrology Institute of Germany).



Analogue temperature probes

Probe type	Dimensions Probe shaft/probe shaft tip	Measuring range	Accuracy	t ₉₉	Order no.
Watertight surface probe with wider measuring tip for plane surfaces, TC type K, fixed cable	0 5 mm Ø 6 mm	-60 to +400 °C	Class 2 1)	30 s	0602 1993
Pipe wrap probe with Velcro strip, for measuring temperatures on pipes with diameters up to max. 120 mm, Tmax +120 °C, TC type K, fixed cable	395 mm 20 mm	-50 to +120 °C	Class 1 1)	90 s	0628 0020
Pipe wrap probe for pipe diameters 5 to 65 mm, with interchangeable measuring head, measuring range briefly up to +280 °C, TC type K, fixed cable		-60 to +130 °C	Class 2 1)	5 s	0602 4592
Replacement measuring head for pipe wrap probe, TC type K	35 mm	-60 to +130 °C	Class 2 1)	5 s	0602 0092
Clamp probe for measurements on pipes, pipe diameters 15 to 25 mm (max. 1"), measuring range briefly up to +130 °C, TC type K, fixed cable		-50 to +100 °C	Class 2 1)	5 s	0602 4692
Precise and fast immersion probe, flexible, watertight, TC type K, fixed cable	Ø 1.5 mm	-60 to +1000 °C	Class 1 1)	2 s	0602 0593
Ultra-fast, watertight immersion/ penetration probe, TC type K, fixed cable	60 mm 14 mm 05 mm Ø 1.5 mm	-60 to +800 °C	Class 1 1)	3 s	0602 2693
Immersion measuring tip, flexible, TC type K	Ø 1.5 mm 500 mm	-200 to +1000 °C	Class 1 1)	5 s	0602 5792
Immersion measuring tip, flexible, TC type K	Ø 1.5 mm 500 mm	-200 to +40 °C	Class 3 1)	5 s	0602 5793
Immersion measuring tip, flexible, for measurements in air/flue gases (not suitable for measurements in smelters), TC type K	Ø 3 mm 1000 mm	-200 to +1300 °C	Class 1 1)	4 s	0602 5693
Watertight immersion/penetration probe, TC type K, fixed cable	114 mm 50 mm 0 5 mm 0 3.7 mm	-60 to +400 °C	Class 2 1)	7 s	0602 1293
Flexible, low-mass immersion measuring tip, ideal for measure- ments in small volumes, such as Petri dishes or for surface meas- urements (e.g. fixed with adhesive tape)	Ø 0.25 mm 500 mm TC type K, 2 m, FEP-insulated thermal wire, temperature-resistant up to 200 °C, oval cable with dimensions: 2.2 mm x 1.4 mm	-200 to +1000 °C	Class 1 1)	1 s	0602 0493
Watertight food probe made of stainless steel (IP 65), TC type K, fixed cable	125 mm 30 mm 0 3.2 mm	-60 to +400 °C	Class 2 1)	7 s	0602 2292

¹⁾ According to standard EN 60584-2, the accuracy of Class 1 refers to -40 to +1000 °C (type K), Class 2 to -40 to +1200 °C (type K), Class 3 to -200 to +40 °C (type K). A probe only ever complies with one accuracy class.



Analogue probes

Probe type	Dimensions Probe shaft/probe shaft tip	Measuring range	Accuracy	t ₉₉	Order no.
Thermoelectric couples					
Thermoelectric couple with TC plug, flexible, length 800 mm, fibreglass, TC type K	800 mm Ø 1.5 mm	-50 to +400 °C	Class 2 1)	5 s	0602 0644
Thermoelectric couple with TC plug, flexible, length 1500 mm, fibreglass, TC type K	1500 mm Ø 1.5 mm	-50 to +400 °C	Class 2 1)	5 s	0602 0645
Thermoelectric couple with TC plug, flexible, length 1500 mm, PTFE, TC type K	1500 mm Ø 1.5 mm	-50 to +250 °C	Class 2 1)	5 s	0602 0646
Comfort probe					
Globe thermometer Ø 150 mm, TC type K, for measuring radiant heat		0 to +120 °C	Class 1 1)		0602 0743

¹⁾ According to standard EN 60584-2, the accuracy of Class 1 refers to -40 to +1000 °C (type K), Class 2 to -40 to +1200 °C (type K), Class 3 to -200 to +40 °C (type K). A probe only ever complies with one accuracy class.

Pitot tubes

Probe type	Dimensions Probe shaft/probe shaft tip	Measuring range	Order no.
Pitot tube, length 500 mm, Ø 7 mm, stainless steel, for measuring flow velocity*	500 mm Ø 7 mm	Measuring range 1 to 100 m/s Operating temperature 0 to +600 °C Pitot tube factor 1.0	0635 2045
Pitot tube, length 350 mm, Ø 7 mm, stainless steel, for measuring flow velocity*	350 mm Ø 7 mm	Measuring range: 1 to 100 m/s Operating temperature: 0 to +600 °C Pitot tube factor: 1.0	0635 2145
Pitot tube, length 1000 mm, stainless steel, for measuring flow velocity*	1000 mm Ø 7 mm	Measuring range: 1 to 100 m/s Operating temperature: 0 to +600 °C Pitot tube factor: 1.0	0635 2345
Straight Pitot tube with integrated temperature measurement, incl. connection hose, length 360 mm	360 mm	Measuring range: 1 to 30 m/s Operating temperature: 0 to +600 °C Pitot tube factor: 0.67 Minimum immersion depth: 150 mm	0635 2043
Straight Pitot tube with integrated temperature measurement, incl. connection hose, length 500 mm	500 mm	Measuring range: 1 to 30 m/s Operating temperature: 0 to +600 °C Pitot tube factor: 0.67 Minimum immersion depth: 150 mm	0635 2143
Straight Pitot tube with integrated temperature measurement, incl. connection hose, length 1000 mm	1000 mm	Measuring range: 1 to 30 m/s Operating temperature: 0 to +600 °C Pitot tube factor: 0.67 Minimum immersion depth: 150 mm	0635 2243

^{*}Connection hose required (order no. 0554 0440) or (order no. 0554 0453)



Accessories

A	a fan dinikal ain malaaiku uushaa	Od
Accessorie	s for digital air velocity probes	Order no.
	escope for testo 440 air flow probes m incl. 90° angle)	0554 0960
Telescope ext flow probes	tension (0.9 m) for testo 440	0554 0990
Other acce	ssories	Order no.
+	Measuring stand for comfort level measurements with standard-compliant positioning of probes (incl. case)	0554 1590
	Combi case for testo 440 and multiple probes	0516 4401
	Service case for volume flow measurement	0516 4900
•	testovent 417 funnel set comprising funnel for plate outlets (Ø 200 mm) and funnel for fans (330 x 330 mm) for incoming/outgoing air	0563 4170
	Flow straightener testovent 417	0554 4172
-	USB mains unit incl. cable	0554 1105

DAkkS calibration certificate (temperature); measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, calibration points 11.3 %RH and 75.3 %RH at +25 °C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane an- emometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane an- emometer, Pitot tube; calibration points 5; 10; 15;			
load capacity 700 hPa (mbar) Connection hose silicone-free for differential pressure measurement, length 5 m, maximum load capacity 700 hPa, (mbar) Control and calibration set for Testo humidity probes, saline solution with 11.3% RH and 75.3% RH, incl. adapter for Testo humidity probes Printer BLUETOOTH®/IRDA printer incl. battery and mains unit Spare thermal paper for printer (6 rolls), measurement data documentation can be read for up to 10 years Calibration certificate (temperature), for air/immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); measuring instruments with air/immersion probe; calibration points 11.3 %RH and 75.3 %RH at +25 °C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); 0520 0005 accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0, 500; 1000; 2000; 4000 lux ISO calibration certificate (luminance) calibration points 0, 500; 1000; 2000; 4000 lux ISO calibration certificate (luminance) calibration points 0, 500; 1000; 2000; 4000 lux ISO calibration certificate (luminance) calibration 0520 0034	Other access	sories	Order no.
Sure measurement, length 5 m, maximum load capacity 700 hPa, (mbar) Control and calibration set for Testo humidity probes, saline solution with 11.3% RH and 75.3% RH, incl. adapter for Testo humidity probes Printer BLUETOOTH®/IRDA printer incl. battery and mains unit Spare thermal paper for printer (6 rolls), measurement data documentation can be read for up to 10 years Calibration certificates ISO calibration certificate (temperature), for air/immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, calibration points 11.3 %RH and 75.3 %RH at +25 °C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (luminance); calibration o520 0033		, , , , ,	0554 0440
Printer BLUETOOTH®/IRDA printer incl. battery and mains unit Spare thermal paper for printer (6 rolls), measurement data documentation can be read for up to 10 years Calibration certificates (temperature), for air/immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); measuring instruments with air/immersion probe; calibration points -20 °C; +60 °C ISO calibration certificate humidity, calibration points 11.3 %RH and 75.3 %RH at +25 °C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3 %RH and 75.3 %RH and 75.3 %RH at +25 °C ISO calibration certificate (pressure); 0520 0006 Calibration certificate (pressure); 0520 0006 SCO calibration certificate (pressure); 0520 0006 Calibration certificate (pressure); 0520 0004 Calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration 0520 0010 Doints 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra-0520 0033	sure measurem	ent, length 5 m, maximum load ca-	0554 0453
BLUETOOTH®/IRDA printer incl. battery and mains unit Spare thermal paper for printer (6 rolls), measurement data documentation can be read for up to 10 years Calibration certificates Socialibration certificate (temperature), for air/ of the property o	probes, saline	solution with 11.3% RH and 75.3%	0554 0660
tery and mains unit Spare thermal paper for printer (6 rolls), measurement data documentation can be read for up to 10 years Calibration certificates ISO calibration certificate (temperature), for air/ immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, calibration points 11.3 %RH and 75.3 %RH at +25 °C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0033	Printer		Order no.
(6 rolls), measurement data documentation can be read for up to 10 years Calibration certificates SO calibration certificate (temperature), for air/ immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); 0520 0211 measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, 0520 0006 calibration points 11.3 %RH and 75.3 %RH at +25 °C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); 0520 0005 accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration 0520 0010 points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra-		·	0554 0621
ISO calibration certificate (temperature), for air/ immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, calibration points 11.3 %RH and 75.3 %RH at +25°C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0001		(6 rolls), measurement data documentation can be read for up to 10	0554 0568
immersion probe, calibration points -18 °C; 0 °C; +60 °C DAkkS calibration certificate (temperature); 0520 0211 measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, 0520 0006 calibration points 11.3 %RH and 75.3 %RH at +25°C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); 0520 0005 accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration 0520 0010 points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra-	Calibration of	ertificates	Order no.
measuring instruments with air/immersion probe; calibration points -20 °C; 0 °C; +60 °C ISO calibration certificate humidity, calibration points 11.3 %RH and 75.3 %RH at +25°C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0003			0520 0001
calibration points 11.3 %RH and 75.3 %RH at +25°C DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25°C BEN at +25°C ISO calibration certificate (pressure); 0520 0005 accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration 0520 0010 points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0033	measuring inst	ruments with air/immersion probe;	0520 0211
hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C ISO calibration certificate (pressure); 0520 0005 accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration 0520 0010 points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra-0520 0033		•	0520 0006
accuracy > 0.6 (% of f.v.) ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0001	DAkkS calibration certificate (humidity); electronic hygrometer; calibration points 11.3% RH and 75.3% RH at +25 °C		0520 0206
emometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate flow, hot wire, vane an- emometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0033		"	0520 0005
emometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate (luminance) calibration points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0033		0520 0004	
points 0; 500; 1000; 2000; 4000 lux ISO calibration certificate (CO ₂ ; CO ₂ probes); calibra- 0520 0033		· · · · · · · · · · · · · · · · · · ·	0520 0034
		, ,	0520 0010
			0520 0033